

ALZHEIMER'S

FOREWORD. *This process is still in the testing phase, because even though it has a high probability of success since it has been designed using the logic of the principles that govern the application of electrical energy in the body, it has been very difficult to obtain patients to observe each of the processes from an engineering school. The worst that can happen when testing a process is that the technique does not cure the disease, but it is IMPOSSIBLE to injure or electrocute the patient with a generator (TENS) that uses a 9-volt battery; the electric chair applied 2,000 volts. Before reading about any of the treatments, you should learn about TENS (Transcutaneous Electrical Nerve Stimulator), which is equivalent to medicine, and see its characteristics by reading the corresponding file contained in this same package, and purchase it online, just making sure that within the "Stimulation Modes" it contains the option: "Normal or Constant." If this treatment does not cure you, you should see your treating physician.*

***** PLEASE, TO TREAT THIS DISEASE USE "THE IMMUNE SYSTEM TREATMENT PROCESS"
INSTEAD OF THIS ONE *****

INTRODUCTION

"When analyzing the systemic characteristics of the brain, the most complex in the universe, I saw that the only way to treat it was in a comprehensive or global manner, without having to decipher the damaged subprocesses involved and their characteristics, which could take me a thousand lifetimes. As time went by, I treated each disease independently, achieving partial success, such as slowing the progression of Parkinson's disease in six years but not stopping the involuntary movement of the limbs; or removing frequent but intense pain in a person with Alzheimer's but without being able to assess its effect on memory loss, or eliminating epileptic seizures in a patient treated with three medications and 221 seizures per month, to less than six in the same period. In the end, I saw that they all coincided in the fundamental aspects of their procedure to cure them and that they could be combined into one, with slight changes. "

The final design was provided by the image showing the resonance curves between the different parts of the brain; that is, the ease with which the electric current penetrates it. From this, it can be seen that the greatest resistance to penetration occurs between both ears, which is why this pad position was discarded from the

final treatment.

I. FIRST WEEK

"It is applied daily for five consecutive days."

FRONT OF THE BRAIN.

PAD SIZE.

- a. ***In the ear canals.*** Use round pads measuring 2 or 2.5 centimeters in diameter, rolled up, as they are easy to insert; 3.5-centimeter round pads can also be used, as they are more common on the market and do not need to be inserted completely—just half or a third of the way into the ear canal, pressing the pad with your finger from outside the ear without touching it.


On the forehead. Use a rectangular pad measuring 4 x 4 or 5 x 5 cm.

CURRENT INTENSITY

At each position, increase the intensity until the person perceives its presence, then decrease it slightly until they no longer feel it or experience pain. This is the ideal intensity for treatment.

TREATMENT PROCESS.

Pad position diagram:

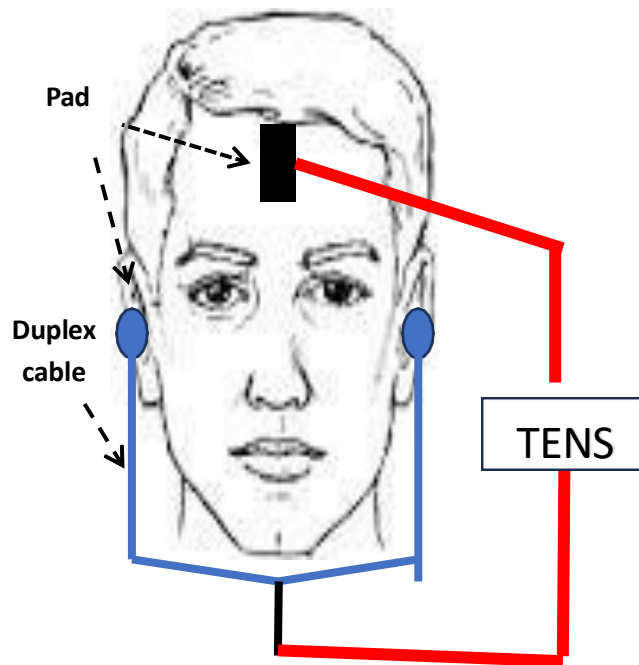

(a)



(b)

**Figure 1a. Pad position in treatment using the frontal suture and auditory pair;
1b. Pads in the center of the forehead using the frontal suture and the nape of**

the neck.

Treatment time:

- a. **Between ears and forehead - 10 minutes.**
- b. **Between forehead and nape of the neck - 10 minutes.**

II. SECOND WEEK.

TREATMENT OF THE CEREBRAL HEMISPHERES

The current always flows from the positive electrode to the negative electrode, i.e., from the red pad to the black pad. In electrical treatment, it does not matter which polarity (positive or negative) is placed on a part of the body; what is relevant for the treatment is that the current crosses the damaged part of the body to heal it. For example, in figure (1.a), a pair of pads are placed in the nostrils using a Duplex cable as shown in figure 3. This forces the current to penetrate both nostrils and ascend through the nasal terminal pair, which penetrates directly into the brain, travels through both cerebral hemispheres, and goes to the two pads placed on the back of the neck using the other Duplex cable covering the entire neck: left, right, and center (Fig. 2).

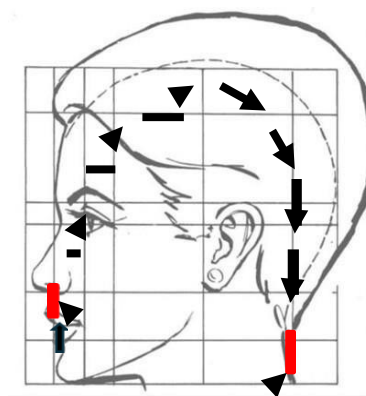


Figure 2. Current path with pads in the left nostril and on the left side of the neck.

This treatment requires two cables as shown in Figure 0.

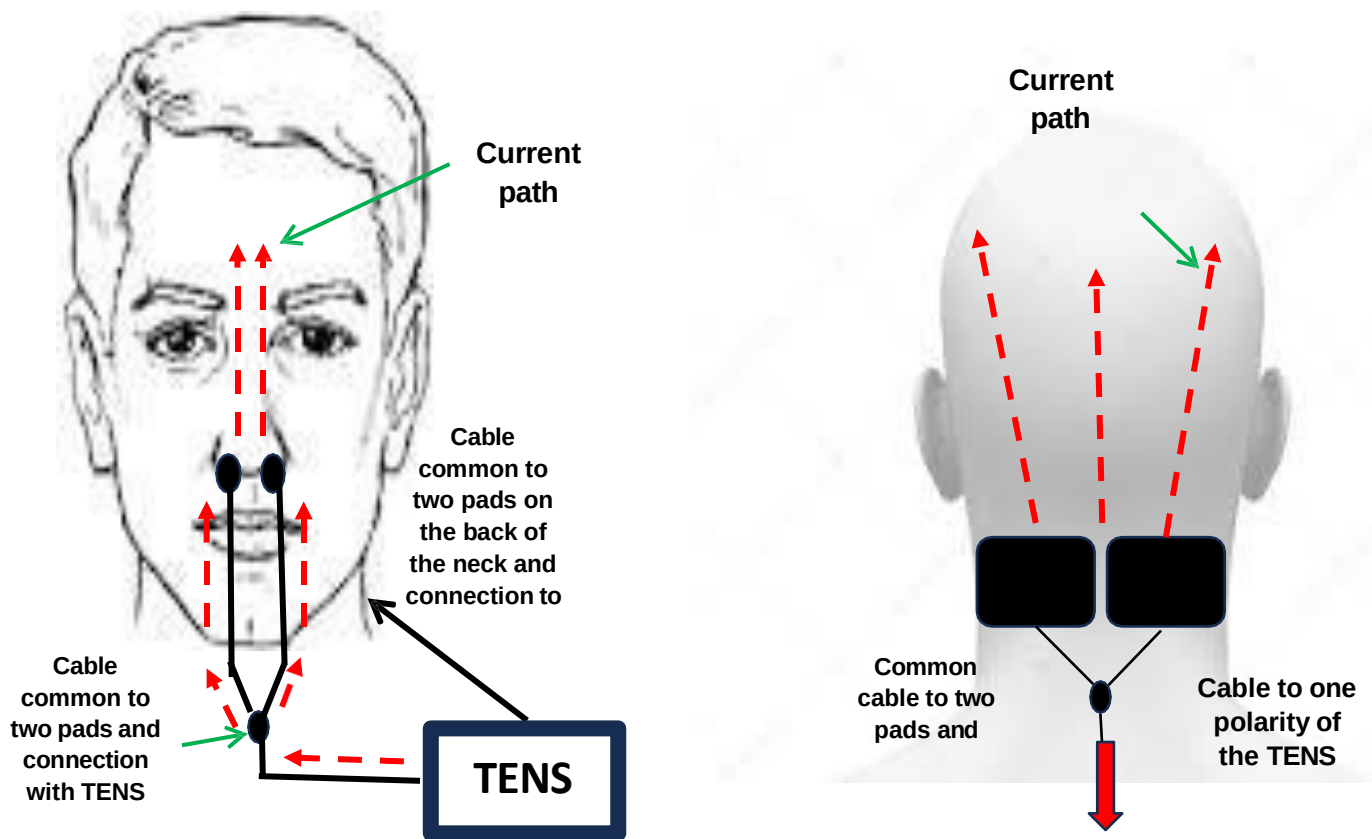


Figure 3. Stimulation of both sides and central part of the brain using the olfactory pairs and two pads on the back of the neck.

TREATMENT:

Current intensity.

As with almost all procedures, increase the current intensity until it is perceived, then lower it very slightly until it is no longer perceived and treat at that position or intensity.

PAD SIZE.


In the nostrils. Use round pads measuring 2 or 2.5 centimeters in diameter, rolled up, as they are easy to insert; 3.5-centimeter round pads can also be used, as they are more common on the market and do not need to be inserted completely—just half or a third of the way into the nostril—and press the pad with your finger from outside the nose without touching it.

On the back of the neck. Preferably use 10 x 5 cm pads to cover the entire width of the back of the neck (it does not matter if the pads touch, as they are connected to the same polarity), but 5 x 5 cm pads can also be used.

Stimulation.

Place a small round pad rolled up in both nostrils and another pair of square or rectangular pads to cover the back of the neck without touching each other, as shown in Figure 3, and stimulate for 20 minutes.

SPINAL TREATMENT

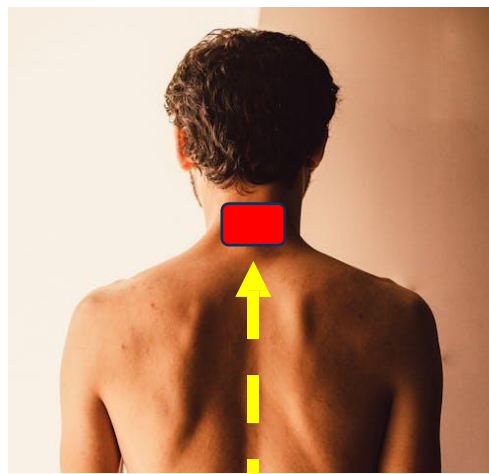

Current intensity.

As with almost all procedures, increase the current intensity until it is felt, then lower it very slightly until it is no longer felt and treat at that position or intensity.

PAD SIZE.

In the nostrils. Use round pads measuring 4 x 8 or 5 x 10 cm.

Treatment time: 10 minutes

Stimulation.

Place a small round pad rolled up in both nostrils and another pair of square or rectangular pads to cover the back of the neck without touching each other, as shown in Figure 3, and stimulate for 20 minutes.

CREATING A CABLE TO CONNECT TWO PADS TO A SINGLE POLARITY

The construction is very simple and the treatment will require two similar cables, which we will call "**Duplex**," made by following the steps below:

1. Obtain a piece of cable and strip it at both ends and in the center, as shown in image 0.

2. Insert each end into the input of both pads.
3. Obtain an alligator clip cable from any electronics store and connect one end to the center of the cable.
4. Connect the other end of the alligator clip to one end of the TENS unit, as shown in figure 0; this will give both pads the same polarity - **Duplex**

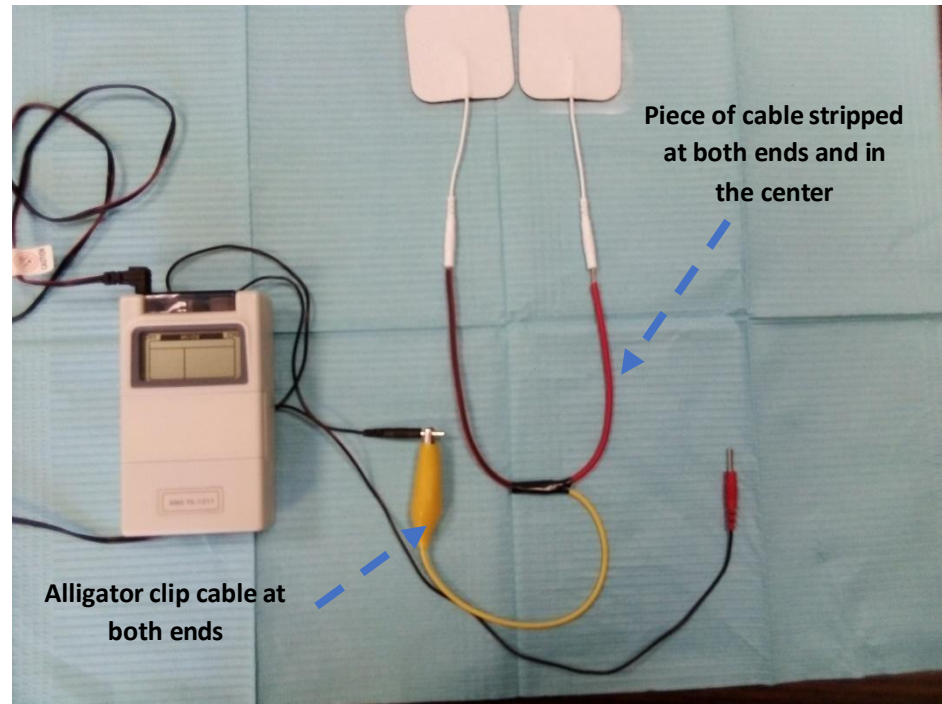


Figure 0. Connection of two pads to the same polarity - Duplex.

