

EPILEPSY

***** PLEASE, TO TREAT THIS DISEASE USE "THE IMMUNE SYSTEM TREATMENT PROCESS"
INSTEAD OF THIS ONE *****

PROLOGUE. *This process has been successfully tested for several years and its effectiveness has been verified. Before reading about any of the treatments, you should learn about TENS (Transcutaneous Electrical Nerve Stimulator), which is equivalent to medicine, and see its characteristics by reading the corresponding file contained in this same package. You can purchase it online, just make sure that the "Stimulation Modes" include the option: "Normal or Constant." If this treatment does not cure you, you should see your treating physician.*

WARNING: *Before reading any of the treatments, you should learn about TENS (Transcutaneous Electrical Nerve Stimulator) and its features: parameter settings, cost, where to buy it, etc., as it is the device that generates the electrical signals used to cure all the diseases shown on this site; it is equivalent to medicine. A description of it is given in the information entitled: "TENS FEATURES" on this same site.*

INTRODUCTION

"When analyzing the systemic characteristics of the brain, the most complex in the universe, I saw that the only way to treat it was in a comprehensive or global manner, without having to decipher the damaged subprocesses involved and their characteristics, which could take me a thousand lifetimes. As time went by, I treated each disease independently, achieving partial success, such as slowing the progression of Parkinson's disease in six years but not stopping the involuntary movement of the limbs; or removing frequent but intense pain in a person with Alzheimer's but without being able to assess its effect on memory loss, or eliminating epileptic seizures in a patient treated with three medications and 221 seizures per month, to less than six in the same period. In the end, I saw that they all coincided in the fundamental aspects of their procedure to cure them and that they could be combined into one, with slight changes. "

The final design was provided by the image showing the resonance curves between

the different parts of the brain; that is, the ease with which the electrical current penetrates it, as shown in the following figure: From this, it can be seen that the

greatest resistance to penetration occurs between both ears, which is why it was ruled out of the final treatment.

CREATION OF A CABLE TO CONNECT TWO PADS TO A SINGLE POLARITY

The construction is very simple and the treatment will require two similar cables, which we will call "**Duplex**," made by following the steps below:

1. Obtain a piece of cable and strip it at both ends and in the center, as shown in image 0.
2. Insert each end into the input of both pads.
3. Obtain an alligator clip cable from any electronics store and connect one end to the center of the cable.
4. Connect the other end of the alligator clip cable to one end of the TENS unit, as shown in figure 0; this will give both pads the same polarity - **Duplex**

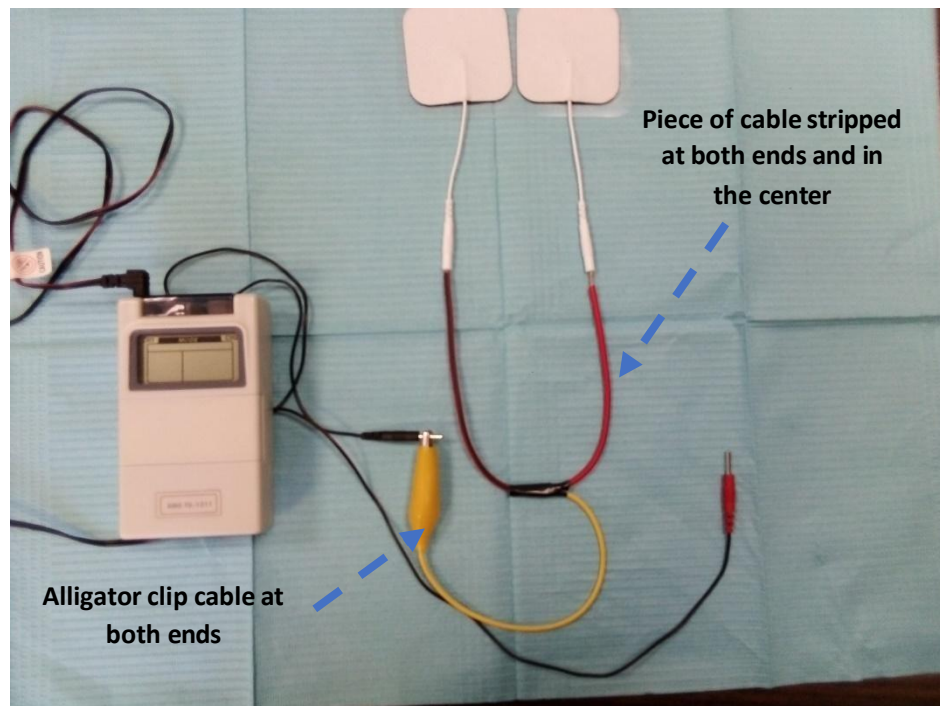


Figure 0. Connecting two pads to the same polarity - Duplex.

I. TWO WEEKS

"Apply daily for ten consecutive days or 5 days in each of the two weeks; Monday through Friday."

FRONT OF THE BRAIN.

PAD SIZE.

- a. ***In the ear canals.*** Use round pads measuring 2 or 2.5 centimeters in diameter rolled up, as they are easy to insert; 3.5-centimeter round pads can also be used, as they are more common on the market and do not need to be inserted completely—just half or a third of the way into the ear canal—and press the pad with your finger from outside the ear without touching it.


On the forehead. Use a rectangular pad measuring 4 x 4 or 5 x 5 cm.

CURRENT INTENSITY

At each position, the intensity is increased until the person feels its presence , and then slightly decreased until it is no longer felt or causes pain. This is the ideal intensity for treatment.

TREATMENT PROCESS.

Pad position diagram:

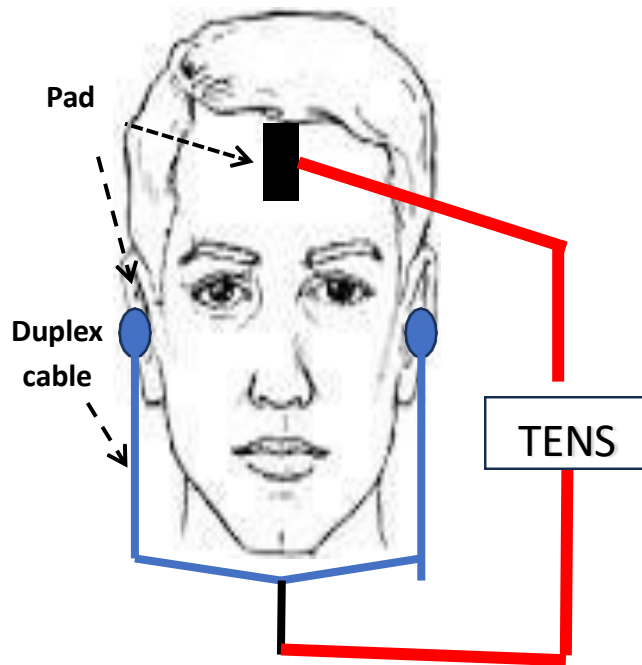

(a)



(b)

Figure 1a. Pad position in treatment using the frontal suture and the auric , 1b.

Pads in the center of the forehead using the frontal suture and the nape of the neck.

Treatment time:

- a. Between ears and forehead - 10 minutes.**
- b. Between forehead and nape of the neck - 5 minutes.**

TREATMENT OF THE CEREBRAL HEMISPHERES

The current always flows from the positive electrode to the negative electrode, that is, from the red pad to the black pad. In electrical treatment, it does not matter which polarity (positive or negative) is placed on a part of the body; what is relevant for the treatment is that the current crosses the damaged part of the body to heal it. For example, in figure (1.a), a pair of pads are placed in the nostrils using a Duplex cable as shown in figure 3. This forces the current to penetrate both nostrils and ascend through the nasal terminal pair, which penetrates directly into the brain, travels through both cerebral hemispheres, and goes to the two pads placed on the back of the neck using the other Duplex cable, covering the entire neck: left, right, and center (Fig. 2).

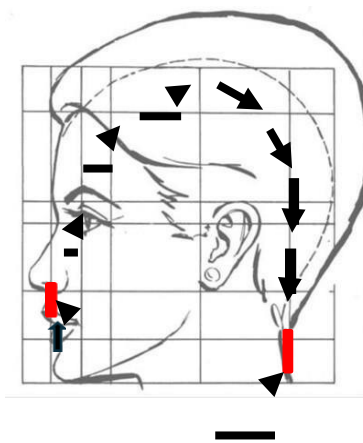


Figure 2. Current path with pads in the left nostril and left side of the back of the neck.

This treatment requires two cables as shown in Figure 0.

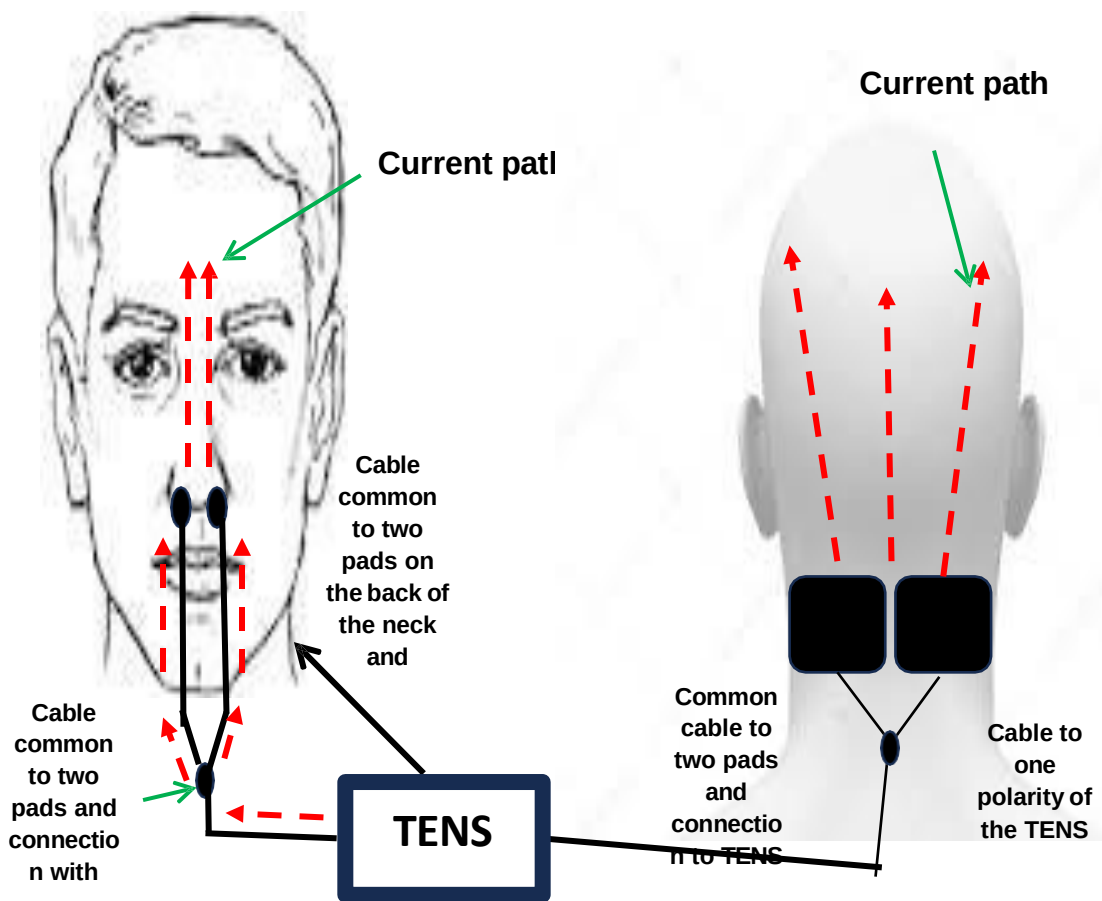


Figure 3. Stimulation of both sides and central part of the brain using the olfactory pairs and two pads on both sides of the back of the neck.

TREATMENT:

Current intensity.

As with almost all procedures, increase the current intensity until it is perceived, then lower it very slightly until it is no longer perceived and treat at that position or intensity.

PAD SIZE.

- b. ***In the nostrils.*** Use round pads measuring 2 or 2.5 centimeters in diameter from rolled up, as they are easy to insert; 3.5-centimeter rounds can also be used, as they are more common on the market and do not need to be inserted completely—just half or a third of the way into the nostril—and press the pad with your finger from outside the nose without touching it.

Stimulation.

Place a small rolled-up round pad in both nostrils and another pair of square or rectangular pads to cover the back of the neck without touching each other, as shown in Figure 3, and stimulate for 20 minutes.

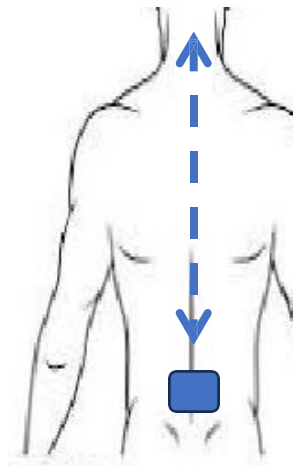


Figure 4. Treatment of the central part of the brain and cerebellum as well as the spinal cord with pads in the nostrils (fig. 3) and another pad at the end of the spine.

Treatment time:

- a. Between nostrils and back of the neck - 15 minutes (fig. 3).**
- b. Between nostrils and end of spine - 5 minutes (fig. 4).**